




FluidInspectIR[®] Portable Ethanol in Gasoline Analyser

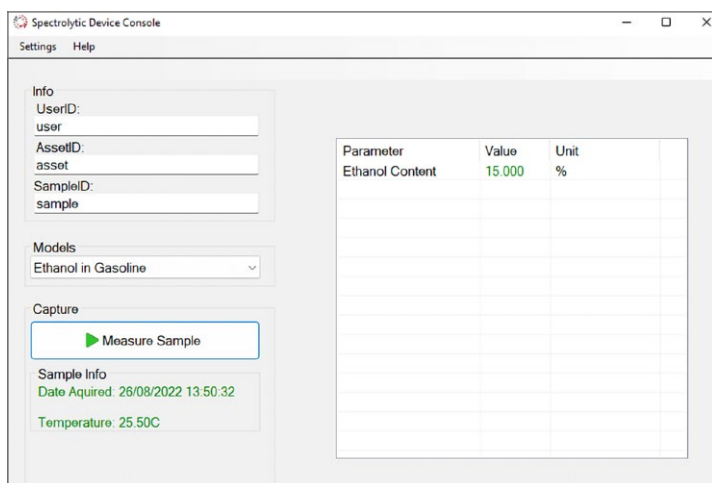

Summary Information

- ▶ Ethanol in Gasoline Analyser
- ▶ Correlates with ASTM D4815(GC)
- ▶ Detectable range of 0 to 20% Ethanol
- ▶ Portable and battery operated

Application

The FluidInspectIR[®] analyser measures the ethanol volumetric % concentration in gasoline samples with the same accuracy as conventional oil laboratories reports.

How to use

The 2-3ml of oil sample is dispensed into the inlet tubing of the flow-cell via a syringe. The flow-cell is placed into the analyser and the measurement is started from the software.

The software is an easy-to-use GUI ran from a Tablet / Laptop (windows 10).

Specification

GUI: Software Console provided for running on windows 10 based laptop / tablet (tablet can be provided as option)

Ambient operating temperature and humidity range: 0-70C non -condensing

Power requirement: 230VAC for mains charging. 2500mAH LiPo battery in device

Internal battery capability typical runtime: 250 sample measurements between charge

Compliance: Correlates with ASTM D4815(GC)

Cuvettes: 1x Cuvettes (flow-cells)

Consumables: Syringes for oil dispense (5ml)

Sample volume: 2-3ml

Repeatability: <+-2% of measured value

Accuracy: <+-2% of measured value

Measurement range: 0 to 20% v/v ethanol in gasoline.

